



# Flow Cryostat - Optical Microscopy

The LT3-OM is designed for optical microscopy and spectroscopy with unique features not found in other cryostats. In addition to the slim 1.52" profile that allows it to fit on most microscope stages. The LT3-OM has a continuously adjustable sample holder, enabling the user to fine tune the placement of the sample within the working distance of their microscopy system.

The LT3-OM vacuum shroud is constructed entirely of welded stainless steel for a cleaner sample environment. The smooth durable stainless steel finish limits the residual vapor pressure of water and reduces the probability of mono layers of water from forming on the sample surface.

The LT3-OM benefits from all of the features that set the ARS manufactured LT3 cryostats apart from other flow cryostats, including the coaxial shield flow transfer line and matrix heat exchanger.

## Applications

- Optical Microscopy
- Micro-Raman
- Quantum Dots
- Photoluminescence
- Micro-Photoluminescence
- Electro-Optical
- Magneto-Optical

## Features

- Continuously adjustable sample height
- Slim 1.52" profile
- Nanometer level vibrations
- Liquid Helium Flow
- Matrix Heat Exchanger
- Co-Axial Shield Flow Transfer Line
- 4K Liquid Helium Operation (1.7K with pumping)
- 0.7 LL/hr liquid helium consumption (tip flow) at 4.2K
- Liquid Nitrogen Compatible (77K Operation)
- Precision Flow Control

## Typical Configuration

- Cold head (LT3OM)
- Coaxial Shield Flow Transfer Line
- Stainless Steel Instrumentation Skirt
- Dewar Adapter
- Flow Meter Panel for Helium Flow Control and Optimization
- Nickel Plated OFHC Copper Radiation Shield Instrumentation for temperature measurement and control:
  - 10 pin UHV feed through
  - 36 ohm thermofoil heater (wire wrapped)
  - Silicon diode sensor curve matched to ( $\pm 0.5K$ ) for control
  - Calibrated silicon diode sensor ( $\pm 12$  mk) with 4 in. free length for accurate sample measurement.
- Flat Plate Sample Holder for Optical Experiments
- Temperature Controller


## Options and Upgrades

- Transmission Upgrade
- Magnet Post upgrade (to fit warm bore of a magnet)
- High Flow Transfer Line
- Custom temperature sensor configuration (please contact our sales staff)
- Custom wiring configurations (please contact our sales staff)
- Sample holder upgrades (custom sample holders available)
- Window material upgrades

DS-LT3OM-R1



The above picture shows LT3OM Helitran®

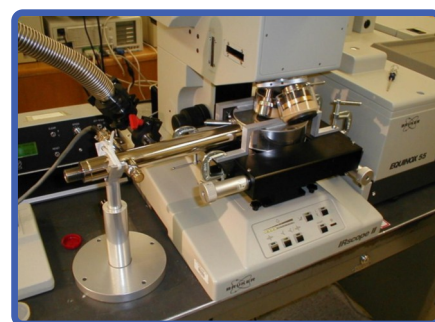



# Flow Cryostat - Optical Microscopy

## Cooling Technology-

LT3-OM	Open Cycle Cryocooler, Helitran
Refrigeration Type	Liquid Helium Flow
Liquid Cryogen Usage	Helium, Nitrogen Compatible

## Temperature\*-

LT3OM	< 4.2K - 350K (<2K with pumping)
With 800K Interface	(Base Temp + 2K) - 700K
With 450K Interface	Base Temp - 450K
Stability	0.1 K
*Based on bare cold head with a closed radiation shield, and no additional sources of experimental or parasitic heat load	

## Sample Space -

Diameter	19 mm (0.75 in)
Height	0-3 mm (0--0.12 in)
Sample Holder Attachment	1/4-28 screw
Sample Holder	<a href="http://www.arscryo.com/Products/SampleHolders.html">www.arscryo.com/Products/SampleHolders.html</a>

## LT3-OM Sample Vibrations- (See Graphs on Page 3)

X-Axis	+/- 5-10 nm
Y-Axis	+/- 5-10 nm
Z-Axis	+/- 5-10 nm

## Temperature Instrumentation and Control - (Standard) -

Heater	36 ohm wire wrapped Thermofoil Heater anchored to the coldtip
Control Sensor	Curve Matched Silicon Diode installed on the coldtip
Sample Sensor	Calibrated Silicon Diode with free length wires
Contact ARS for other options	

## Instrumentation Access-

Instrumentation Skirt	Bolt On, Stainless Steel
Pump out Port	1 - NW 25
Instrumentation Ports	1
Instrumentation Wiring	Contact sales staff for options

## Radiation Shield -

Material	Nickel Plated OFHC Copper
Attachment	Bolt On
Optical Access	1 or 2

## Cryostat Footprint -




Overall Length	562 mm (22.12 in)
----------------	-------------------

Cryostat Model	LT3-OM		
Cryogen	Liquid Helium		Liquid Nitrogen
Base Temperature	4.2K	<2K with Pumping	77K
Nominal Helium Consumption at 4.2K	0.7 LL/hr	-	
Cooling Capacity	0.7 LL/hr	2 LL/hr	
	4.2K		
	0.5W	1.5W	
	20K	8.0W	
	50K	20W	
Maximum Temperature	450K with cold gas through transfer line		
Cooldown Time	20 min		
Weight	0.9 kg (2 lbs)		



# Flow Cryostat - Optical Microscopy


## LT3-OM Drive and Vibration Levels (X, Y, & Z Axis)

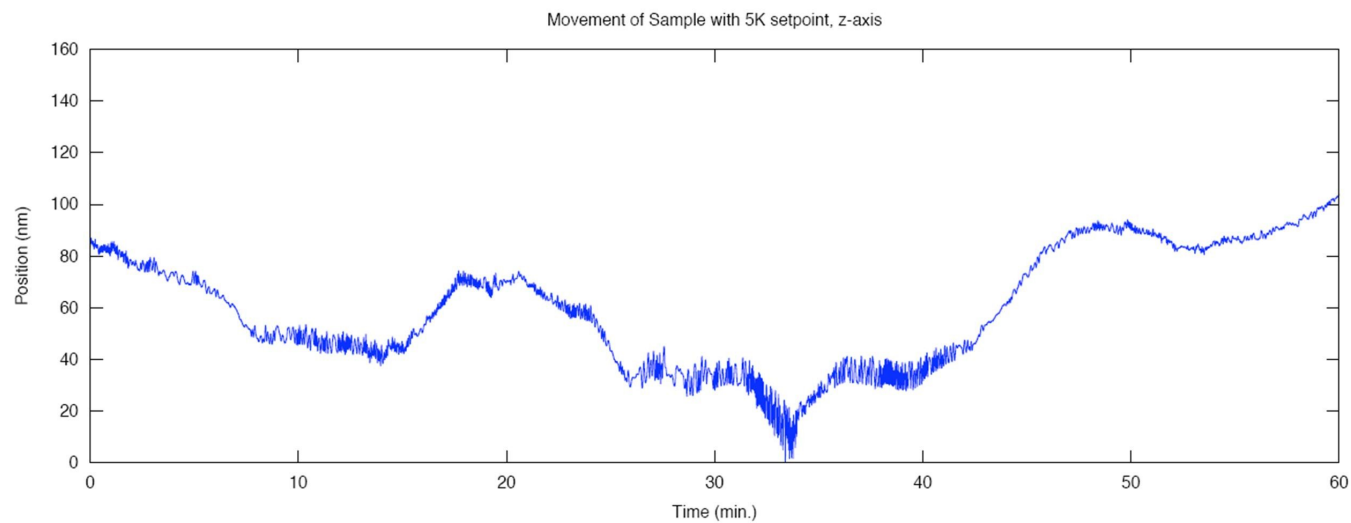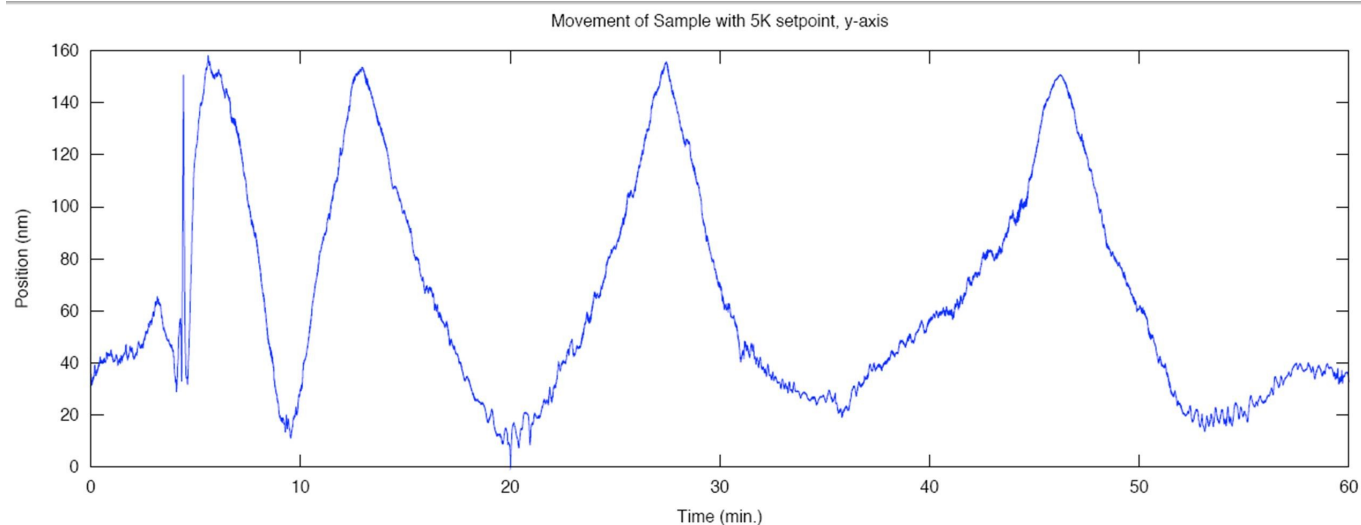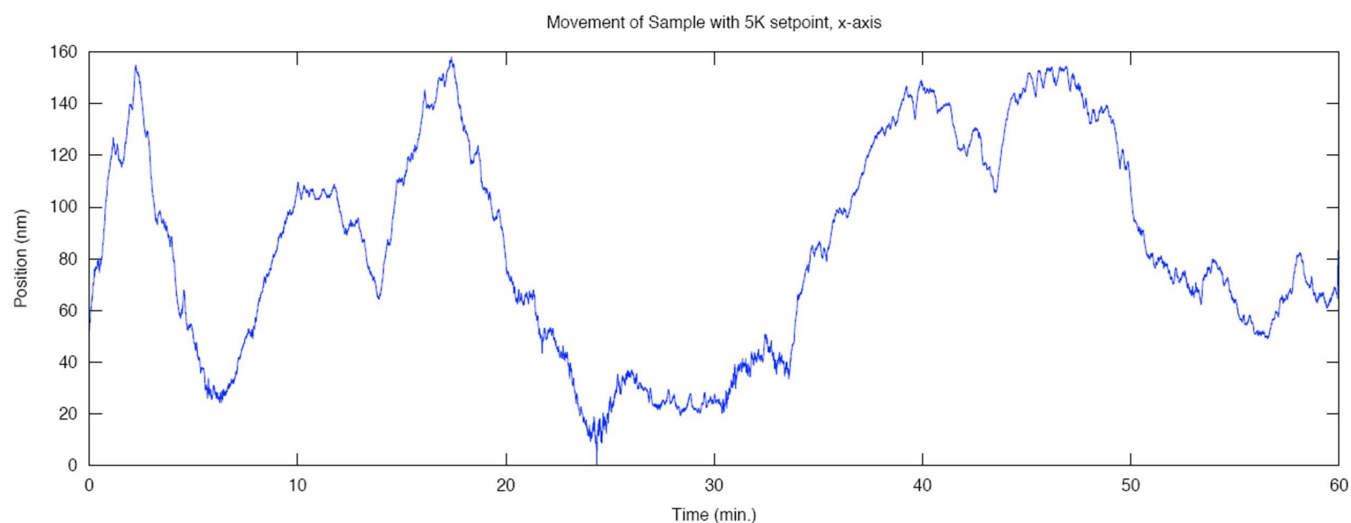



# Flow Cryostat - Optical Microscopy

**LT3OM Outline Drawing**

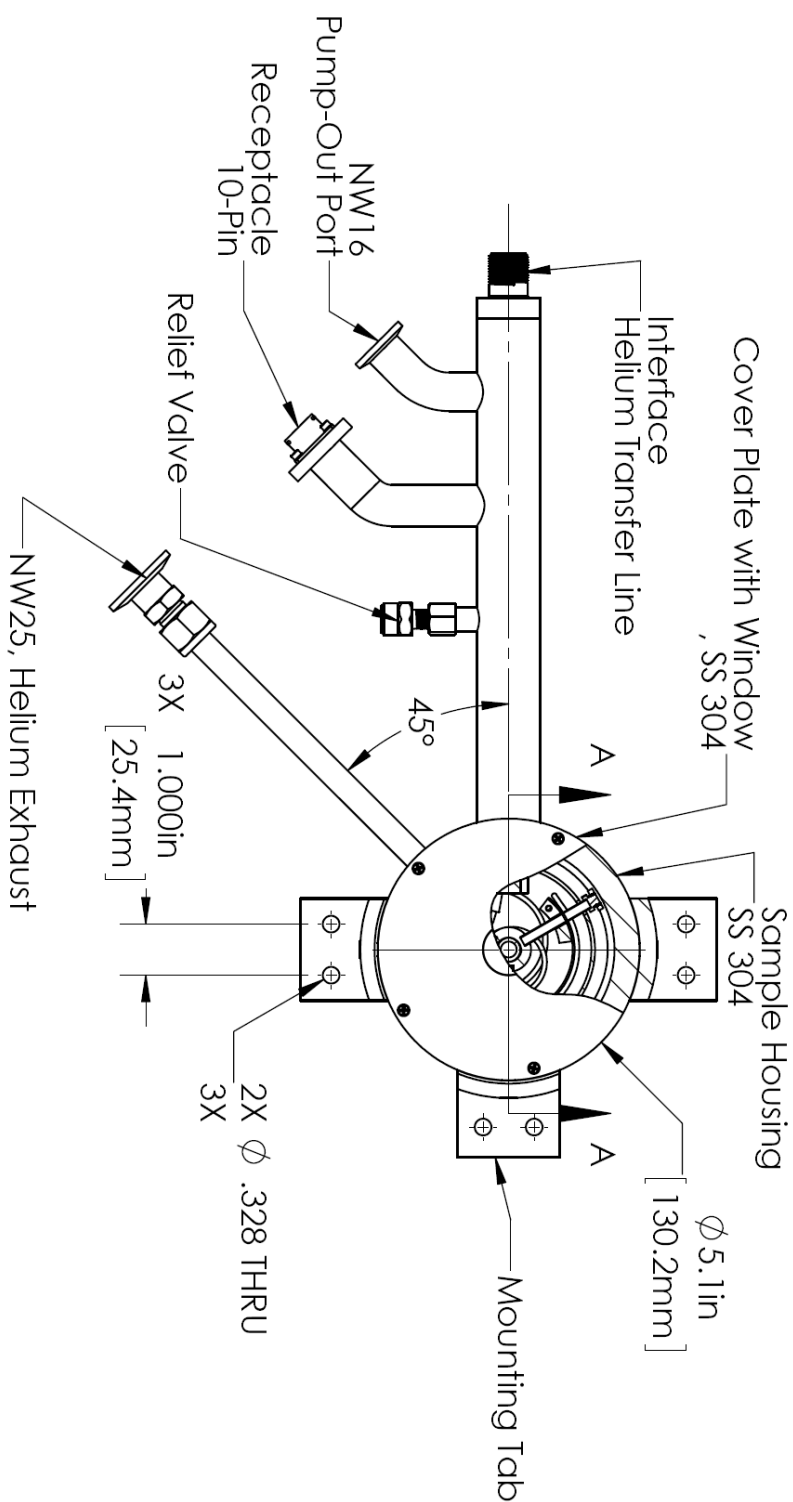



# Flow Cryostat - Optical Microscopy

## Advanced Features of LT3 Helitran®

The Helitran® has been designed for high performance with advanced features not normally found in traditional open cycle cryostats. A detailed description of the **Matrix Heat Exchanger**, the **Adjustable Impedance Valve** and the **Coaxial Transfer Line** is presented in this paper

### Helium Consumption:

Conventional Helium Flow Cryostats do not incorporate extended surface Heat Exchangers (at the sample mount) for cost reasons. The liquid helium is contained in a reservoir similar to a copper cup over the sample mount. As the helium boils and evaporates only the latent heat of vaporization is used to cool the sample mount, there is no provision to capture the enthalpy of the gas as it escapes from the cryostat at 4.2K regardless of the sample temperature. The cooling power of the gas is wasted. Enthalpy of Helium gas from 4.2 to 300K is substantial at 1542 Joules/gm.

The Helitran® incorporates an extended surface tip heat exchanger (**Matrix Heat Exchanger**) which provides efficient heat transfer between the helium and the sample mount. The Liquid helium flows through this heat exchanger and as the latent heat of vaporization cools the sample mount, the liquid evaporates, the gas continues to flow through the exchanger providing additional cooling (capturing the enthalpy of the gas) to the sample mount. If the flow is optimized the helium gas will exit the Matrix Heat Exchanger at a temperature equal to the sample temperature.

Helium usage is dramatically reduced as reported by J. B. Jacobs in Advances in Cryogenic Engineering, Volume 8, 1963, Page 529 as follows:

Amount of Cryogenic fluid required to cool metals (Liters/Kg.) to 4.2K.


Cryogen	<sup>4</sup> He	<sup>4</sup> He
Initial Temperature of 1 Kg of Copper.	300K	77K
Final Temperature of 1 Kg of Copper,	4.2K	4.2K
Using the latent heat of vaporization only. <b>(Inefficient Heat Transfer)</b>	<b>31.1</b> Liters of Helium	2.16 Liters of Helium
Using the Enthalpy of Gas. <b>(Efficient Heat Transfer)</b>	<b>0.79</b> Liters of Helium	0.15 Liters of Helium

From this it is clear that for any sample size the consumption of He during initial cooldown is 40 times higher without an extended surface cryostat tip heat exchanger from 300K (room temperature) to 4.2K and 14 times higher when cooling from 77K to 4.2K.

### Temperature Range:

**Sub 4.2K Operation:** The temperature of helium drops to 1.8K when the pressure is reduced across an **Adjustable Impedance Valve**. Pumping on a reservoir, as in a traditional system is not practical as all the helium will evaporate rather quickly. In the Helitran® the suction is applied against the Impedance Valve by attaching a vacuum pump, this reduces the pressure of the helium as it flows through the Matrix Heat Exchanger, The matrix heat exchanger and the conductively coupled sample mount are cooled to below 1.8K.

**800K Operation:** The high temperature can be achieved by incorporating a thermal switch, composed of a sapphire and OFHC copper arrangement as shown below. The unique property of sapphire is utilized, where its thermal conductivity is equal to that of copper from 4-300K but it becomes a thermal insulator above 300K. The high cooling power of the Matrix Heat exchanger protects the cryostat.

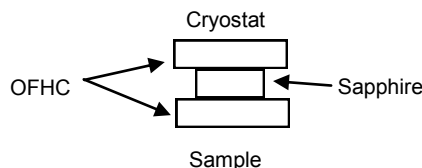

### Temperature Stability:

Conventional helium flow cryostats utilize a capillary tube in a vacuum jacket with superinsulation to reduce the radiant heat load. However as the helium absorbs radiant heat the liquid is vaporized and forms bubbles of gas which have a larger volume than the liquid thus forming a temporary block to the flow of the liquid called "vapor binding". At the delivery end of the transfer line this results in the liquid/gas mixture being delivered in spurts with accompanying pressure and temperature cycling.


The coaxial flow transfer line incorporates a shield flow (See figure) surrounding the tip flow for the entire length of the transfer line. The entrance to the coaxial shield flow tube is provided with a nozzle which results in a pressure and corresponding temperature drop in the shield flow which subcools the tip flow in the center tube. This subcooling prevents boiling and gas bubble formation in the helium, even at very low flow rates. The Helium is delivered at the sample end with the desired temperature stability and low vibrations.



# Flow Cryostat - Optical Microscopy

## Cryostat Design Features


### Helitran® Continuous Flow Cryostat.

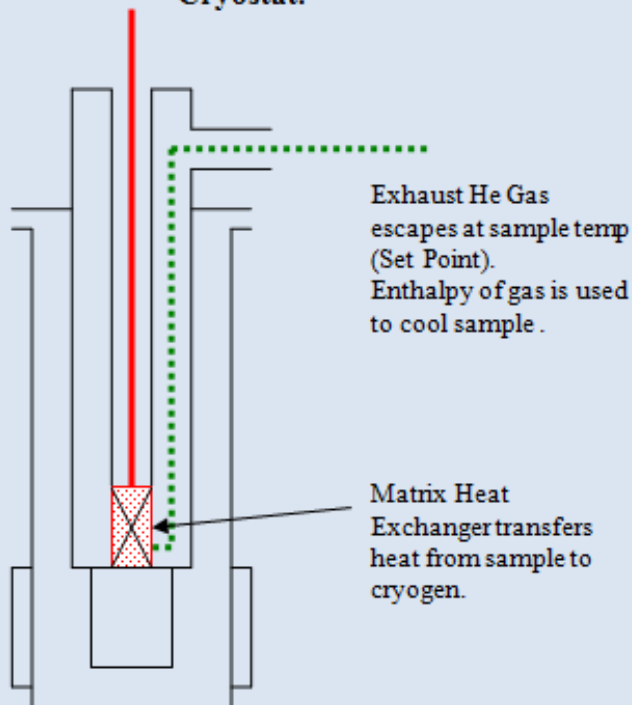

#### Helitran® Features:

- Matrix Heat Exchanger for efficient heat transfer between sample mount and cryogen.
- Orientation independent.

### Conventional Continuous Flow Cryostat

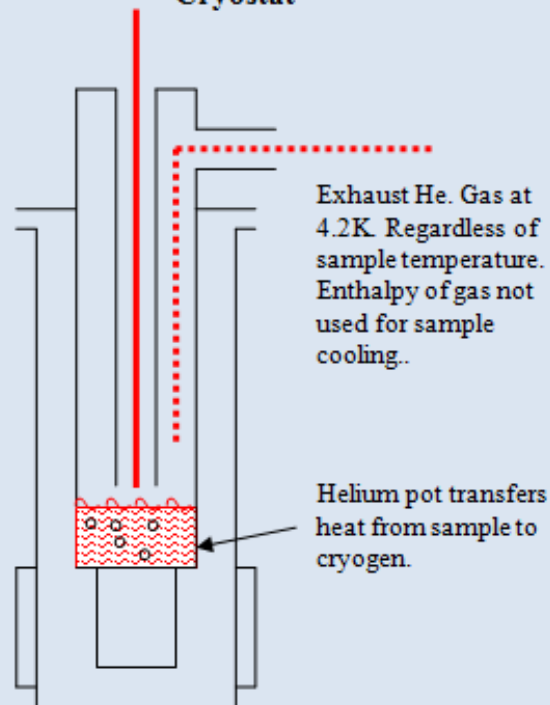

#### Conventional Helium Flow Cryostat Features:

- Helium reservoir exchanger results in helium boiling with resulting vibrations from the bubbling.
- Orientation dependent as helium is gravity contained.
- Gas escapes at 4.2K. No provision for heat transfer between sample mount and Helium gas from 4.2K to the sample temperature.



# Flow Cryostat - Optical Microscopy

## Helium Flow Transfer Line Features

